trulyclear
ULTRASONIC LIGHT THERAPY

trulyclear Ultrasonic Light Therapy Skin Renewal System

Ultrasound/Phototherapy/Ionotherapy

User Manual

Please read this manual carefully before using your new **trulyclear Ultrasonic Light Therapy Skin Renewal System**

Recommended for home and personal use only
Not for treatment of medical conditions

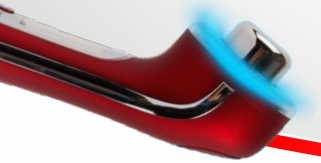

trulyclear
ULTRASONIC LIGHT THERAPY

Introduction

Congratulations on purchasing your new trulyclear Ultrasonic Light Therapy Skin Renewal System. Please read the information included in this user manual for complete instructions on getting the most from your system. Keep the manual handy for future reference.

The revolutionary trulyclear Ultrasonic Light Therapy Skin Renewal System is an advanced Photon Galvanic Rejuvenation System that includes a skin renewal device designed for home use that is safe, effective and easy to use. Prepare to experience real gain with no pain as you employ our revolutionary system.

The trulyclear Ultrasonic Light Therapy Skin Renewal System will deliver phenomenal results with minimum effort on your part. The only scientifically proven home device that actually produces dramatic results, the trulyclear Ultrasonic Light Therapy Skin Renewal System stimulates your body's own healing powers to heal damaged skin, reduce the appearance of fine lines and wrinkles, firm, smooth and restore a youthful radiance.

Powered by cutting edge, Ultrasonic Light Therapy technology, the trulyclear Ultrasonic Light Therapy Skin Renewal System focuses three highly-effective light beams deep into the dermis. The trulyclear Ultrasonic Light Therapy technology stimulates dermal activity, tightening collagen fibers and spurring new collagen production. Skin becomes firmer and more supple, lines and wrinkles are reduced and the effects of the aging process are virtually reversed, for every type and color of skin.

- An effective alternative to surgery, Botox and chemical peels
- A proven, relaxing treatment in the privacy of your own home
- Scientific, clinical proof of a high level of success for long-lasting effects
- Safe and effective for all skin types and skin colors

Find a new you……today!!

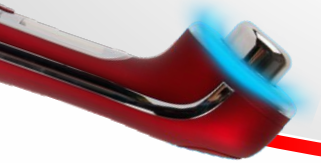

trulyclear
ULTRASONIC LIGHT THERAPY

Contents

Safety Notice, Precautions	4
Package Contents	4
Device Controls & Features	4
Benefits by function	5
How to use device functions	6
What to expect	9
Device Care and Maintenance	9
Troubleshooting	9
Specifications	10
Warranty	11

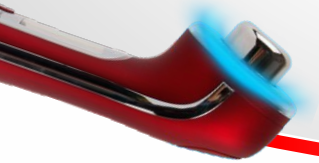

trulyclear
ULTRASONIC LIGHT THERAPY

Important Safety Notice

- Do not disassemble or modify the device as this may cause device damage, malfunction, electrical shock, fire or personal injury. There are no user-serviceable parts inside the device.
- Keep the trulyclear Ultrasonic Light Therapy Skin Renewal System out of reach of children.
- Do not expose trulyclear Ultrasonic Light Therapy Skin Renewal System to open flame.
- Do not use the trulyclear Ultrasonic Light Therapy Skin Renewal System in or near water and store in a dry location.
- Dropping the trulyclear Ultrasonic Light Therapy Skin Renewal System device may cause irreparable damage.
- Unplug docking base when not in use (on applicable models only).

Precautions

Do not use this device If you are currently under medical care for a skin condition, consult your doctor before using the trulyclear Ultrasonic Light Therapy Skin Renewal System.

The trulyclear Ultrasonic Light Therapy Skin Renewal System is designed for personal use only by a single user.

Use the protective goggles provided with the trulyclear Ultrasonic Light Therapy Skin Renewal System.

Do not look directly at the light source of the treatment head of this device while it is in operation.

Stop immediately, if you experience any adverse effect or have a concern regarding use. Contact your doctor. You may be having a photosensitive reaction.

Package Content

- trulyclear Ultrasonic Light Therapy Skin Renewal System device
- Power Supply Adapter/Charger
- Goggles
- Cotton pad
- Cotton pad holder

Device Controls and Features

HQ stainless steel
3M HZ Ultrasonic ION (Galvanic) microwave massage head

Therapy Lights:
Red LED: 625+/-3nm
Blue LED: 465+/-3 nm
Green LED: 525+/-3nm

Function LCD Display

Power On/Off Button

Mode Button

Shift Button

Confirm Button

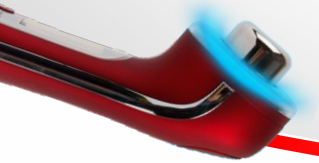

trulyclear
ULTRASONIC LIGHT THERAPY

Benefits by Function

The trulyclear Ultrasonic Light Therapy Skin Renewal System provides a wide array of benefits, including:

- Helps to heal and clear acne and other skin conditions
- Reduces the appearance of fine lines, wrinkles, and scarring
- Renews skin, firms, smoothes, increases skin's capacity to absorb nutrients and moisture

Skin Rejuvenation-Ultrasound Therapy

- Red LED Light: Promotes the reduction of blemishes, softens skin and reduces the appearance of fine lines and wrinkles, firms and increases the production of collagen.
- Blue LED Light: Effective in diminishing inflammation, eliminating bacteria that causes acne and healing acne and other scarring.
- Green LED Light: targets and breaks up melanin clusters that cause skin discoloration resulting in luminous and radiant skin.
- Ultrasonic -The ultrasonic function of the trulyclear Ultrasonic Light Therapy Skin Renewal System massages skin and increases cell efficiency, stimulating the healing power of the cytomembrane, increasing the permeability of the skin while raising the overall temperature of deep layers of skin to promote absorption of nutrients, accelerate metabolism and reinforce the regenerative processes in tissue. Besides its regenerative abilities, ultrasonic also works to decompose waste in the surrounding fat as well as aiding in the repair of lymph and capillary vessels.
- Soothing Microwave Massage applies a safe and pleasant vibrating microwave massage at a frequency of 12,000 rpm to the deep dermis effectively cleanses the skin, softening the residue of cosmetics in pores to facilitate cleaning, breaks up oils, reduces the incidence of blackheads and clogged pores and helps to facilitate the discharge of skin oils.
- Galvanic (ION+ ION-): The Galvanic function has two operating modes; (ION+) and (ION-). The ION+ positive mode cleanses the skin by attracting oil, dirt and other impurities from deep inside pores and removes them from your skin. The ION- negative mode infuses nutrients deeper into the dermis and activates the cell renewal process. It also increases the effectiveness of your serums and moisturizers.

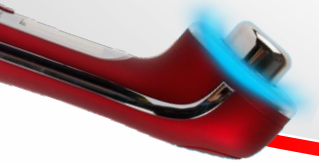

trulyclear
ULTRASONIC LIGHT THERAPY

How to Use Device Functions

Getting Started

1. Make sure the trulyclear Ultrasonic Light Therapy Skin Renewal System device is plugged into an electrical socket for electrical power devices. Make sure the trulyclear Ultrasonic Light Therapy Skin Renewal System portable rechargeable device is fully connected to the charger and charged before using. The device will take approximately 3 hours to charge. You may charge your device by connecting it to the charger and connecting the charger to an electrical wall socket, or you may connect it to your computer using a USB cord and USB port. An indicator on the LCD display is shown when charging and turns off when device is fully charged.
2. Remove the protective film from the head of the trulyclear Ultrasonic Light Therapy Skin Renewal System prior to using.
3. Before using on face, test an area of skin on your wrist for sensitivity, following the directions for use. If swelling, reddening, itching, pain or other unusual reactions occur, discontinue use. If the condition persists, call your doctor.
4. Cleanse your skin thoroughly to remove all makeup or creams from the area to be treated.
5. Turn the power on for the trulyclear Ultrasonic Light Therapy Skin Renewal System using the power indicator button on the device handle and follow instructions for desired treatment. For rechargeable devices, make sure the device is fully charged. For electrical devices, make sure the device's cord is connected to an electrical outlet.

Skin Rejuvenation: Anti-Aging/Anti-Acne/Anti-Pigmentation

Red, Blue or Green Light Therapy + Ultrasonic
Begin the treatment by placing the ultrasonic probe of the device against your skin, with the complete surface of the head in contact with the skin (do not allow the device head to tip so that only part of it is in contact with skin. Make sure it is fully in contact with skin. Slowly glide the device over the area to be treated moving device in circular motions. Treatment time is 3 minutes per treatment area.

Photofacial treatment cycles should be performed 3 to 4 time a week for the first 2 months, then once or twice a week to maintain results.

*** Do Not look directly at the light source of the treatment head while it is in operation. During photon therapy, it is recommended to wear the included eye goggles to protect the eyes. (Looking directly at the LED light application may cause discomfort, dizziness and possible injury to eyes.)**

1. Press POWER button to power ON device.
2. Press MODE button, the ULTRASONIC indicator will flash, press SHIFT to select intensity level (there are 5 levels, select a comfortable level between 1 and 5).

3. Press CONFIRM
4. Press MODE button, until you see PHOTON indicator flashing, press SHIFT to select, RED, BLUE or GREEN light therapy (Select Red, Blue or Green according to desired treatment.)
5. Press CONFIRM.
6. Press MODE button, until you see the TIME indicator flash, press SHIFT to select 3 minutes. (Note: Treatment time is 3 minutes per treatment area. However, if you are treating more than one area, you can set the timer for additional minutes. Example: 3 treatment areas X 3 minutes = 9 minutes.)
7. Press CONFIRM and device will begin operation. (Note: The device can be interrupted during the treatment cycle by pressing CONFIRM button once and restarted by pressing CONFIRM button again.)

Skin Cleansing

Galvanic (ION+)

Begin the treatment by placing the ultrasonic probe of the device against your skin, with the complete surface of the device probe head in contact with the skin (do not allow the device probe head to tip so that only part of it is in contact with skin. Keep treatment area moist by using a cotton ball or cotton pad lightly moistened with water. Make sure the device probe head is fully in contact with skin. Slowly glide the device over the area to be treated moving device in circular motions. Treatment time is 4 minutes per treatment area. Rinse face with water after treatment.

Galvanic treatment cycles should be performed 5 times a week for the first 2 months, then 2 to 3 times a week to maintain results.

1. Press POWER button to power ON device.
2. Press MODE button , the ULTRASONIC indicator will flash, press SHIFT button to select intensity level (there are 5 levels, select a comfortable level from 1 to 5).
3. Press CONFIRM button
.4. Press MODE button, until you see CLEAN+ indicator flashing, press SHIFT button to select intensity level (there are 5 levels, select a comfortable level from 1 to 5).
5. Press CONFIRM button.
6. Press MODE button until you see RELAX indicator flashing, press SHIFT until you see MICROWAVE MASSAGE indicator flashing.
7. Press CONFIRM button.
8. Press MODE button, until you see the TIME indicator flashing, press SHIFT button to select 4 minutes
9. Press CONFIRM button and device will begin operation. (Note: The device can be interrupted during a treatment cycle by pressing CONFIRM button once and restarted by pressing CONFIRM button again).

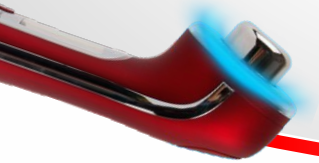

trulydear
ULTRASONIC LIGHT THERAPY

Galvanic (iON+) Nourish Skin

Clean your skin thoroughly, rinse well and pat dry with a soft cloth. Begin the treatment by placing the ultrasonic probe of the device against your skin, with the complete surface of the device probe head in contact with the skin (do not allow the device probe head to tip so that only part of it is in contact with skin. Make sure the device probe head is fully in contact with skin. Slowly glide the device over the area to be treated moving device in circular motions. Treatment time is 4 minutes per treatment area. After treatment, apply your favorite skincare products, as your skin is better prepared to absorb skin moisturizing products.

Galvanic treatment cycles should be performed 5 times a week for the first 2 months, then 2 to 3 times a week to maintain results.

1. Press POWER button to power ON device.
2. Press MODE button , the ULTRASONIC indicator will flash, press SHIFT button to select intensity level (there are 5 levels, select a comfortable level from 1 to 5).
3. Press CONFIRM button.
4. Press MODE button, until you see NOURISH- indicator flashing, press SHIFT button to select intensity level (there a 5 levels, select a comfortable level from 1 to 5).
5. Press CONFIRM button.
6. Press MODE button until you see RELAX indicator flashing, press SHIFT until you see MICROWAVE MASSAGE indicator flashing.
7. Press CONFIRM button.
8. Press MODE button, until you see the TIME indicator flashing, press SHIFT button to select 4 minutes.
9. Press CONFIRM button and device will begin operation. (Note: The device can be interrupted during a treatment cycle by pressing CONFIRM button once and restarted by pressing CONFIRM button again).

LCD Display Settings

Battery charge indicator for rechargeable devices

Ultrasonic Level Indicator (1 to 5 levels)

Galvanic Level Indicator (1 to 5 levels)

Galvanic Ion indicator for ION+ (Positive) for skin cleansing function, and ION – (Negative) for nutrition absorption and infusing serums or moisturizers.

Relax indicator for micro-vibration massage, including continuous and pulse modes.

Photon indicator for red light, blue light and green light treatments

Time indicator for time set, from one (1) to fifteen (15) minutes

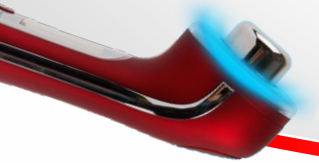

trulyclear
ULTRASONIC LIGHT THERAPY

What to Expect

DURING TREATMENT:
Some users will experience skin redness and minor swelling which is expected immediately after the treatment and is a natural part of the healing process. Both will disappear within a few moments. Many users experience an increase in hydration and skin plumping immediately.

AFTER 1 WEEK OF TREATMENT:
Most users will start to see an improvement in skin texture while the majority of users will see an increase in the healthy feel of their skin and an increase in skin smoothness.

AFTER 2 WEEKS OF TREATMENT:
A vast majority of users will see a reduction in the overall signs of aging, particularly an increase in skin firmness.

AFTER 4 WEEKS OF TREATMENT:
Many users will see overall better skin condition compared to before treatment. This includes an improvement in the healthy appearance of the skin and a reduction in fine lines and wrinkles.

In a clinical study, proven results showed a 30 percent reduction in fine lines, a 16 percent reduction in wrinkling within three (3) to four (4) weeks. In addition, overall skin texture was greatly improved. (Note - These results differ in some people, and depend on the individual skin characteristics of each.)

Device Care and Maintenance

The following maintenance instructions are important to ensure that your device continues to work as it was designed. Failure to follow these instructions may cause your device to stop delivering the required dose and to stop functioning altogether. Make sure to Power OFF your device before cleaning.

Battery Care: It is recommended to keep your device fully charged. You may charge your device by connecting it to the charger and connecting the charger to an electrical wall socket, or you may connect it to your computer using a USB cord and USB port. An indicator on the LCD display is shown when charging and turns off when device is fully charged.

Cleaning: The treatment head should be cleaned following each use. Your device is not waterproof. DO NOT submerge in the device in water, doing so will result in permanent damage and void any product warranty. Use a damp, soft. lint-free cloth and a mild alcohol-free detergent to clean the treatment head surface. Repeat with water only. Dry surface using a clean dry cloth.

Troubleshooting

If your trulyclear Ultrasonic Light Therapy Skin Renewal System does not work properly, please try these common maintenance tasks before contacting us at: support@trulyclearskin.com

For Electrical Models:

- Make sure the power cord is properly connected at the device and at the wall socket.
- Make sure the power to the device is ON.
- Make sure the proper function is selected according to the instructions in this manual.
- If the power cord is damaged, contact us at support@trulyclearskin.com for a replacement.
- If you have not selected any operation to begin within 30 seconds, the device will automatically shut down to protect the circuitry.

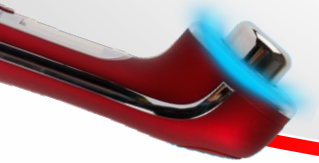

For Rechargeable Models:

- Make sure the device is completely charged to full capacity.
- Make sure the device is turned ON and the LCD display light is ON.
- If the display is not lit, the built-in lithium battery may be low. Try charging the device to full capacity (about 3 hours).
- If the battery indicator light is flashing, it indicates that the built-in lithium battery is low. Charge the device to full capacity (about 3 hours).
- If you have not selected any operation to begin within 30 seconds, the device will automatically shut down to protect the circuitry.

Specifications

Product Information

Name/Model Number:
trulyclear Ultrasonic Light Therapy System/ tc89070405

Manufacturer:
Accelebrite, subsidiary of Million Dollar Smile

Operating Specifications

Ambient Temperature:
40 - 100 degrees Fahrenheit

LED Information

Red	625± 3nm
Green	525± 3nm
Blue	465± 3nm
Ultrasonic:	3MHz
Galvanic:	ION +/ ION - HQ Stainless Steel Head

Power Supply

Input-Power Cord Device:	AC100-240V 50/60HZ; Output: DC15V, 0.4A
Input-Rechargeable Device:	AC100-240V 50/60HZ; Output: DC5.0 V 1.0A
Li-ion battery:	1100 mAh
Charging Time:	Approximately three (3) hours for rechargeable devices
Electrical power supply classification:	Class II-double insulation
Weight:	150 g. (electrical device) 165 g. (rechargeable device)
Size:	Height 2 inches/ Length 7.3 inches / Width 2 inches

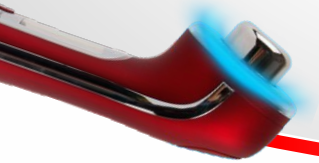

trulyclear
ULTRASONIC LIGHT THERAPY

Warranty

Register Your Device at www.trulyclearskin.com/warranty

Your trulyclear Ultrasonic Light Therapy Skin Renewal device is warranted to be free from defect in material and workmanship for a period of one year after its original purchase date under normal use. This warranty extends only to the original retail purchaser with original proof of purchase and only when purchased from an authorized retailer or reseller of Million Dollar Smile products.

If the product should become defective within the warranty period, contact: support@trulyclearskin.com for repair or replacement. If you are outside of North America, contact your local distributor. Million Dollar Smile LLC reserves the right to replace a defective product with the most comparable product currently available. Your exclusive remedy for any defective product covered by this limited warranty is limited to the repair or replacement of the defective product. Million Dollar Smile LLC's entire liability for any defective product shall in no event exceed the purchase price for the defective product

This warranty does not cover products determined by Million Dollar Smile LLC to be damaged by any of the following:

Accident, misuse, abuse or alteration
Servicing by unauthorized persons
Use with unauthorized accessories or use other than as instructed
Connecting to incorrect current and voltage
Any other conditions beyond our control

TO THE EXTENT PERMITTED BY LAW, Million Dollar Smile LLC. SHALL NOT BE RESPONSIBLE FOR ANY DIRECT OR INDIRECT DAMAGES RESULTING FROM THE USE OR MISUSE OF THIS PRODUCT INCLUDING ANY GENERAL, INCIDENTAL, SPECIAL, OR CONSEQUENTIAL DAMAGES. ALL IMPLIED REPRESENTATIONS, WARRANTIES OR CONDITIONS INCLUDING BUT NOT LIMITED TO ANY IMPLIED REPRESENTATIONS, WARRANTIES OR CONDITIONS OF FITNESS AND MERCHANTABILITY ARE LIMITED IN DURATION TO ONE YEAR FROM DATE OF ORIGINAL PURCHASE.

This warranty gives you specific legal rights, and you may also have other rights that vary depending on your state, province or other jurisdiction. Some jurisdictions do not allow the exclusion or limitation of incidental or consequential damages, or limitations on how long an implied warranty lasts, so the above limitations and exclusions may not apply to you.

trulyclear
ULTRASONIC LIGHT THERAPY

san diego california
support@trulyclearskin.com